we analyzed over

2,700

SAMPLES



from


2,000

## **BREATH COLLECTIONS**


at partner clinics and customers, plus our in-house research and development samples.

This was A YEAR-ON-YEAR \$\frac{1}{2}\$

INCREASE

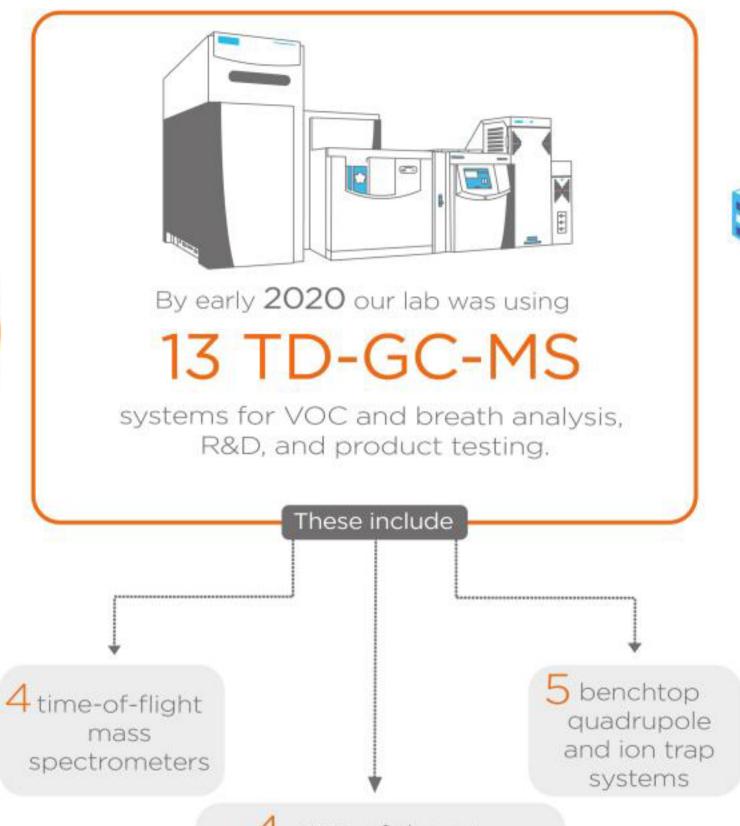

4 state-of-the-art
Thermo Scientific™
Q Exactive™ Orbitrap™
Mass Spectrometers
plus one more on order

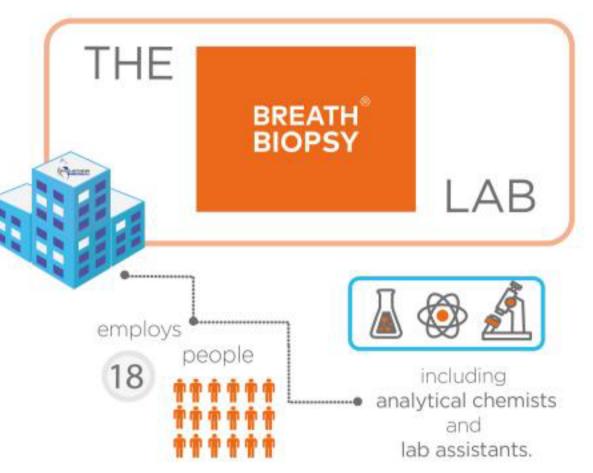



## The lab supplies CLEANED AND TESTED



Breath Biopsy Cartridges for clinics and customers.





We currently have around

10,000

tubes in circulation, managed through an in-house database.